

FIG. 1

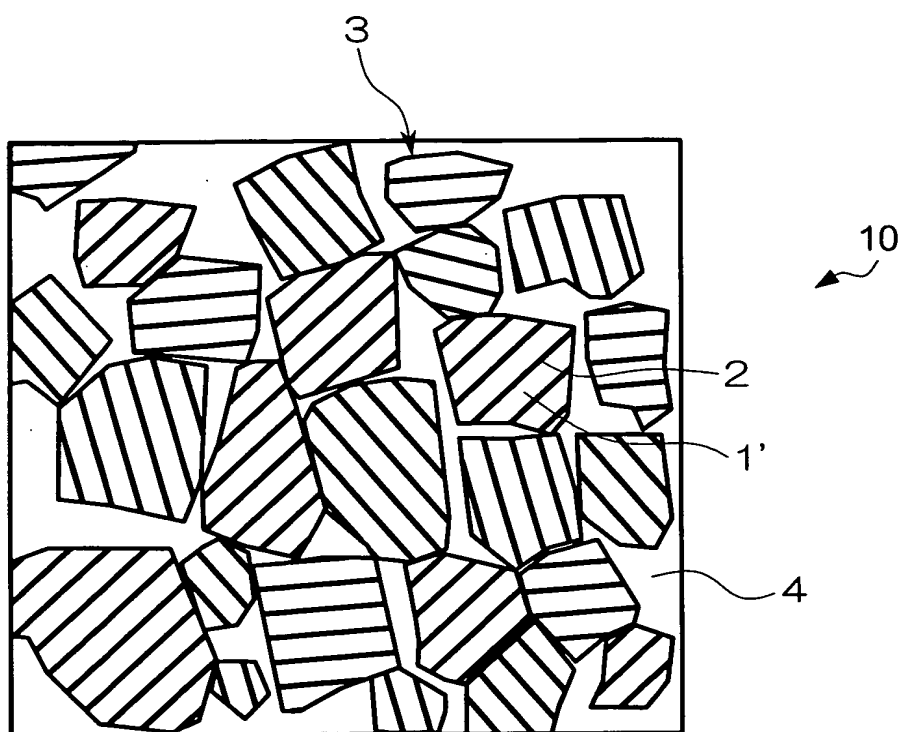


FIG. 2



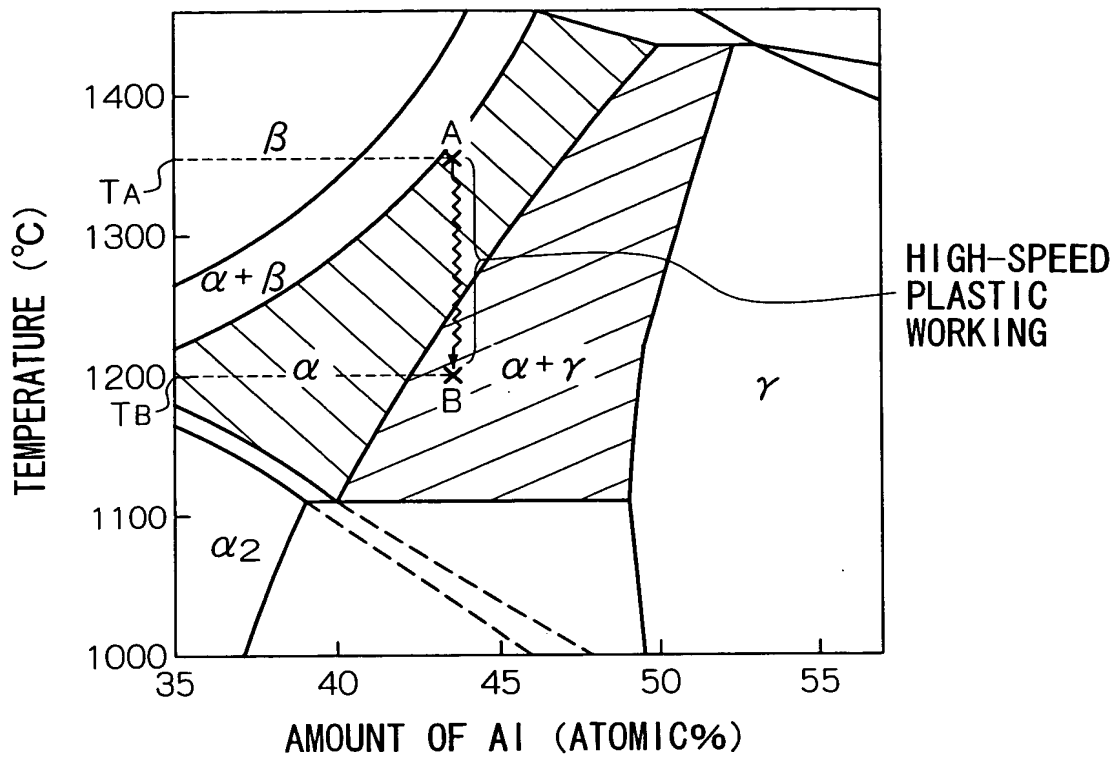


FIG. 3A

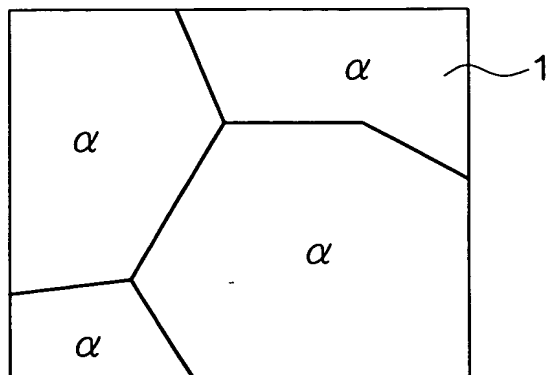

STEP A

FIG. 3B

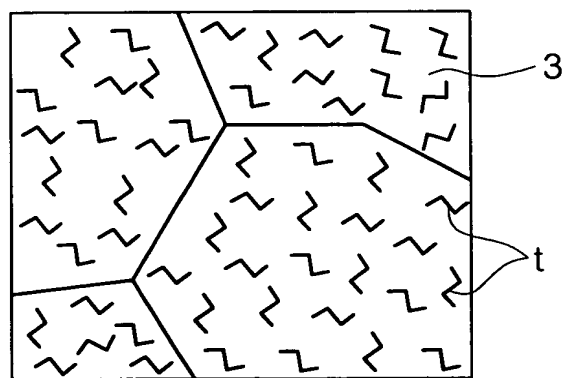

STEP B

FIG. 3C

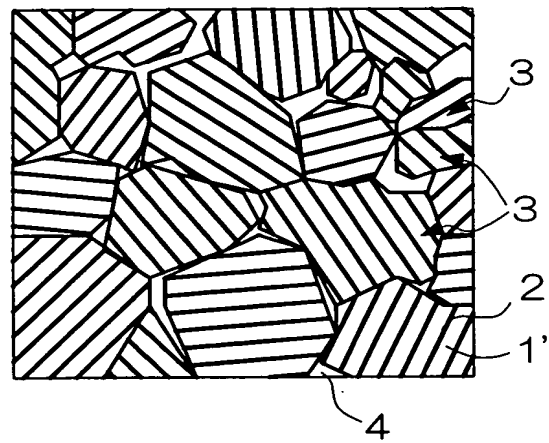
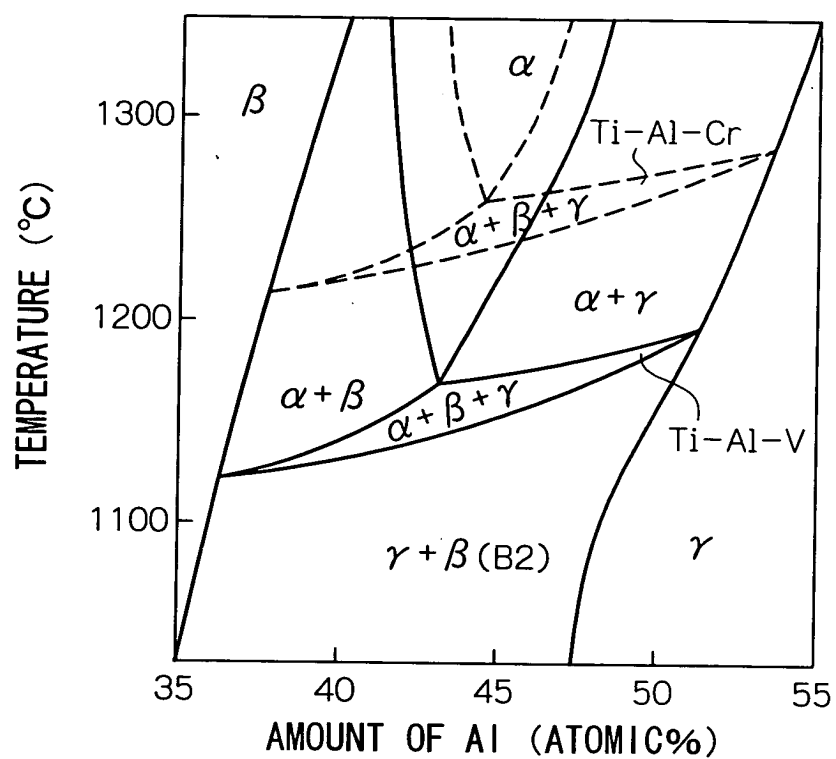


FIG. 4



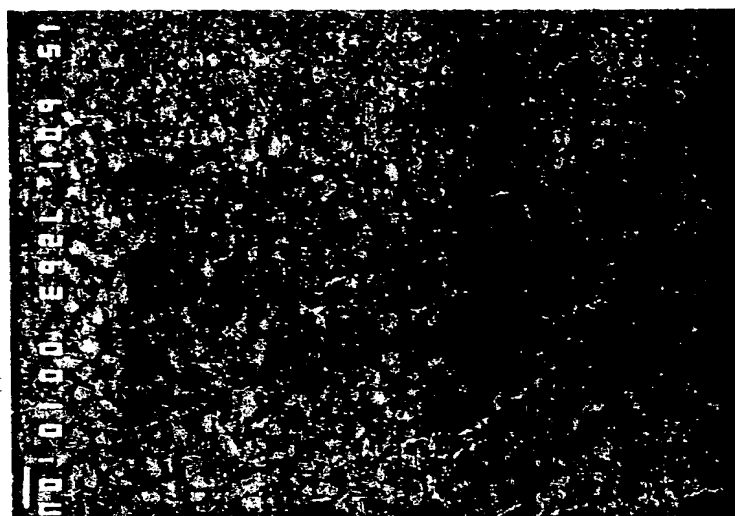


FIG. 5

20 μ m

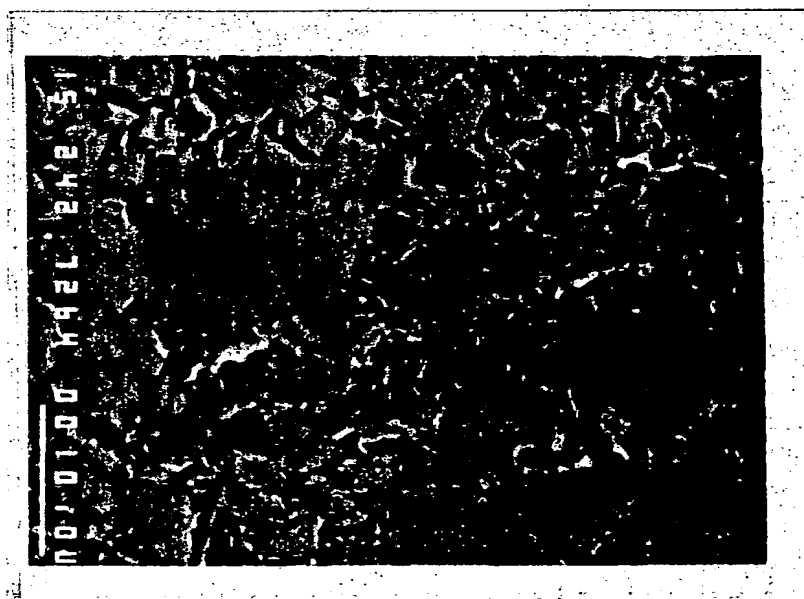


FIG. 6

5 μ m

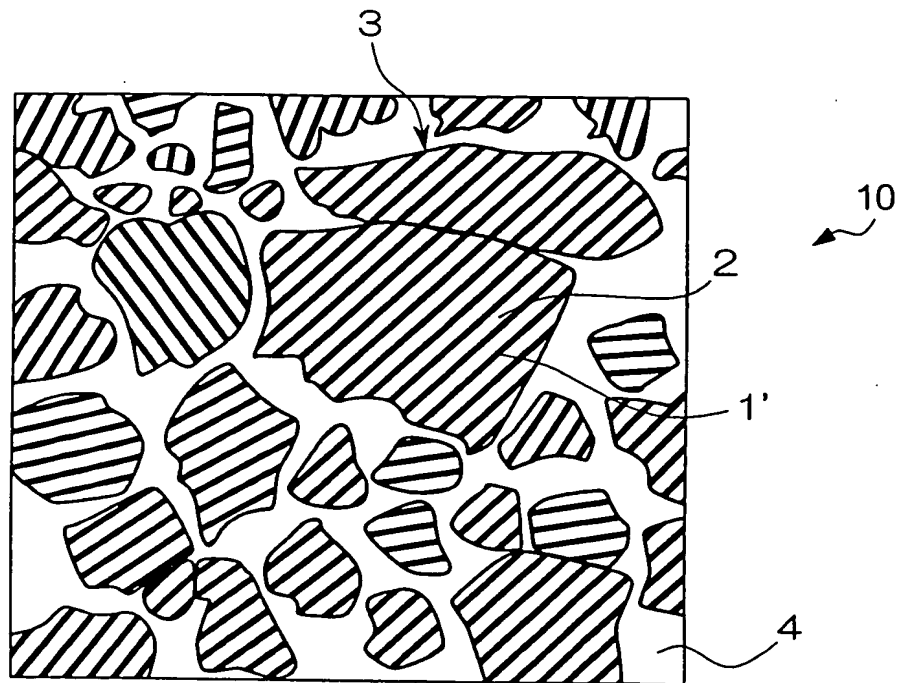


FIG. 7

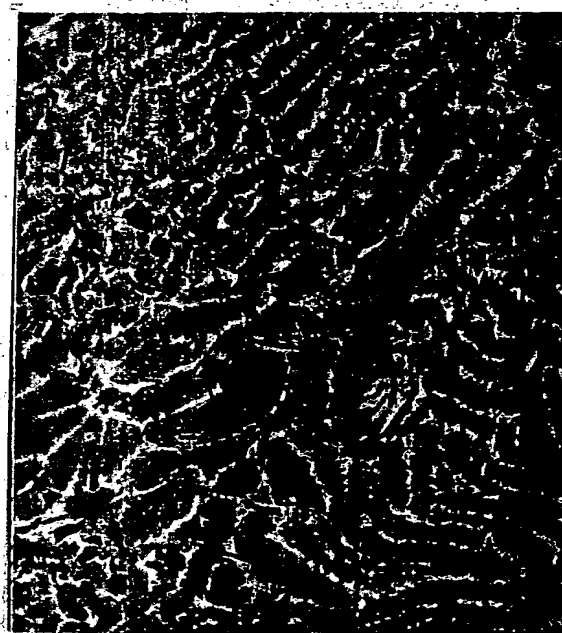


FIG. 8

10 μm

FIG. 9A



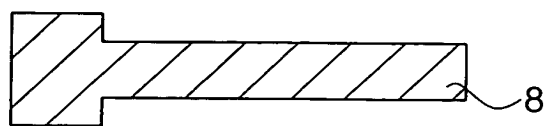


FIG. 9B

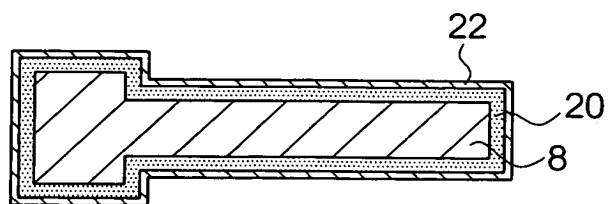

STEP A'

FIG. 9C

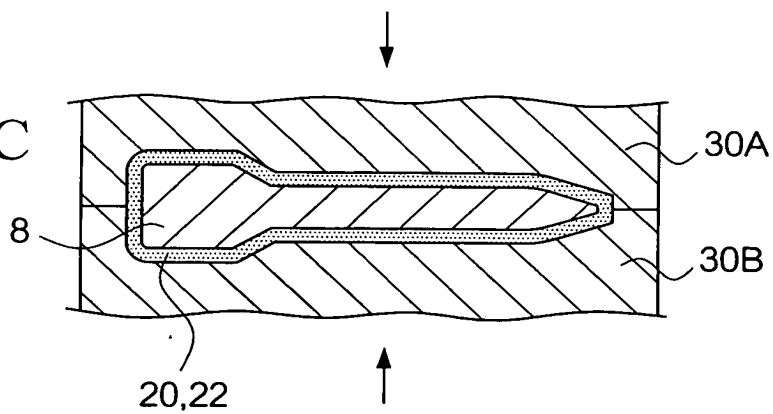

STEP B'

FIG. 9D

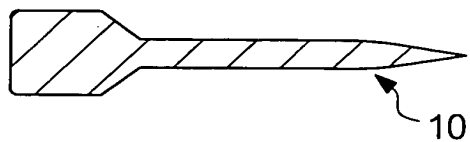
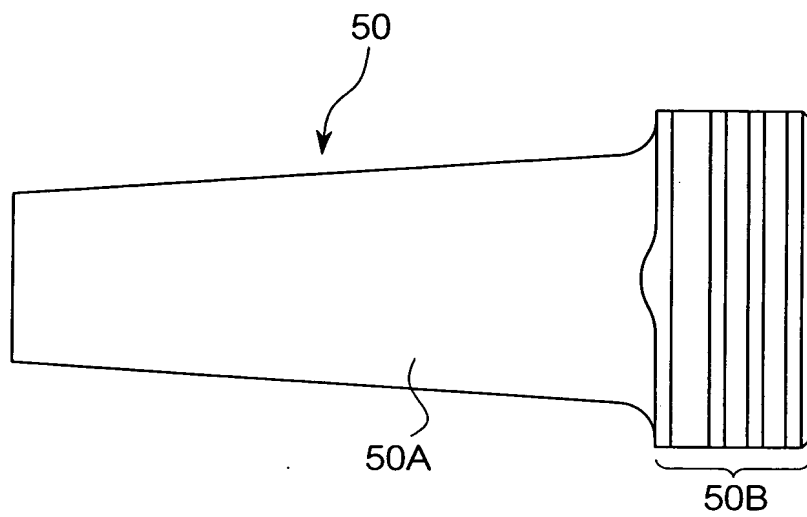


FIG. 10



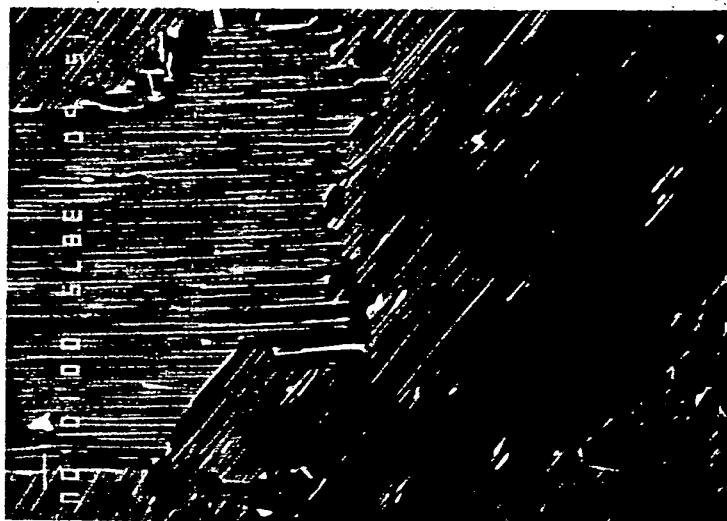


FIG.11

20 μ m



FIG.12

5 μ m